

## IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re Patent of:	)	
	:	Examiner: Brett Alan Crouse
AKIHITO SAITOH ET AL.	)	
	:	Art Unit: 1774
Appln. No.: 10/506,300	)	
	:	
Filed: September 1, 2004	)	Confirmation No.: 8354
	:	
For: OLIGOFLUORENLYLENE COMPOUNDS	)	
	:	
U.S. Patent No.: 7,229,702 B2	)	
	:	
Issued: June 12, 2007	)	January 9, 2008

Commissioner for Patents  
P.O. Box 1450  
Alexandria, VA 22313-1450

LETTER CALLING ATTENTION TO ERRORS IN PATENT

Sir:

The following minor errors have been noted in the above-mentioned patent:

ON COVER PAGE AT (54) TITLE

“OLIGOFLUORENLYENE” should read --OLIGOFLUORENYLENE--.

COLUMN 1


Line 12, “emit” should read --emits--.

COLUMN 4


Line 57, “ditolyaminopheynyl” should read --ditolylaminophenyl--.

COLUMN 47

Structure 91a-d, “

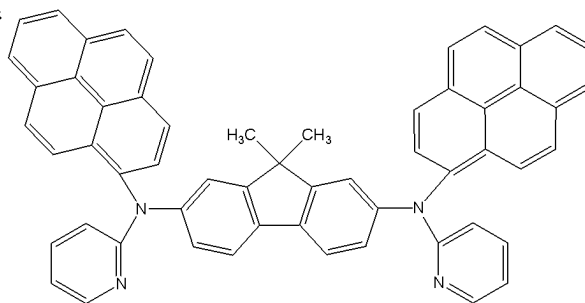

should read

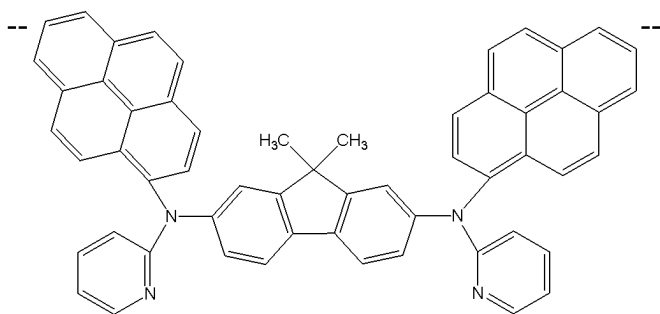

COLUMN 75

Lines 40-43, delete the sentence beginning with “This type of liquid-emitting device is” and ending with “use in the device”.


COLUMN 76

Line 53, “providing a” should read --providing an--.

COLUMN 78

Line 1-20, “


”

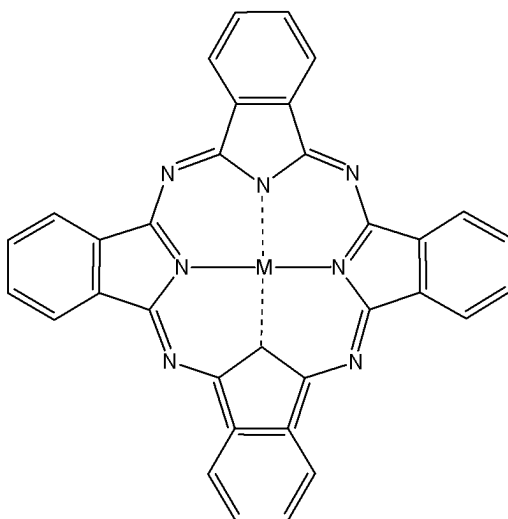

should read


--

--.

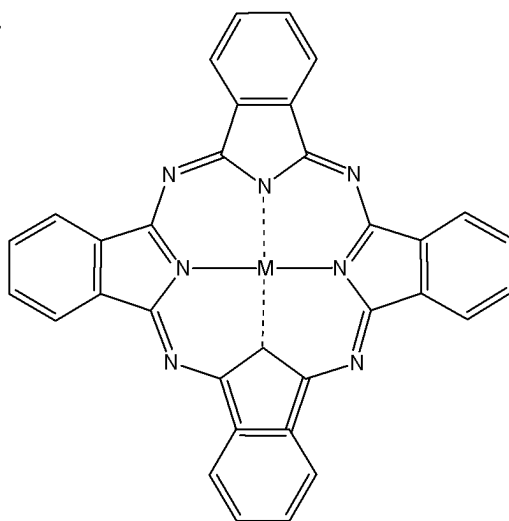


COLUMN 85

Line 45-52, “

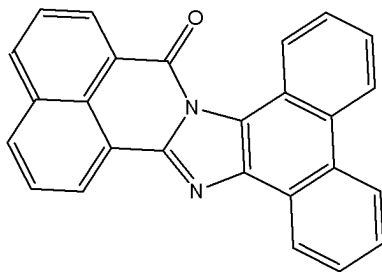

should read

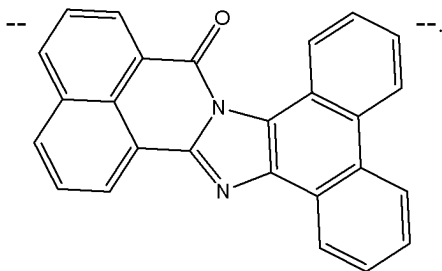

COLUMN 89

Line 50, “Poly thiophene” should read --Polythiophene--.

These errors appear to be relatively insignificant and, therefore, have not been included in the Certificate of Correction which has been filed separately. However, it is requested that this paper be placed in the filewrapper of the above-identified patent.

Patentees' undersigned attorney may be reached in our New York office by telephone at (212) 218-2100. All correspondence should continue to be directed to our address given below.

Respectfully submitted,

/Peter Saxon /  
Peter Saxon  
Attorney for Patentees  
Registration No. 24,947

FITZPATRICK, CELLA, HARPER & SCINTO  
30 Rockefeller Plaza  
New York, New York 10112-3801  
Facsimile: (212) 218-2200